LUMEX® by graham-field

7016A: STAINLESS STEEL 4-HOOK IV STAND ASSEMBLY AND OPERATION INSTRUCTIONS

SAVE THESE INSTRUCTIONS FOR FUTURE USE

Tools required: *M8 hex key, M6 hex key (included)*

Info: *The most current version of these instructions can be found online at www.grahamfield.com.*

⚠ **WARNING: Important! Read and understand these instructions before assembling or using the Stainless Steel 4-Hook IV Stand. If you do not understand any part of these warnings or instructions, contact a healthcare professional for direction in the use of this product. If the IV Stand is not properly assembled, personal injury and damage to the IV Stand could result.**

⚠ **WARNING: If components are damaged or missing, contact your GF distributor immediately. DO NOT use substitute parts. Use only Lumex replacement parts. Non-Lumex replacement parts could cause personal injury and damage to the IV Stand.**

⚠ **WARNING: GF Health Products, Inc. assumes no responsibility for any damage or injury caused by improper assembly, installation or use of this product.**

INTENDED USE

The intended use of the Stainless Steel 4-Hook IV Stand is the suspension of IV and other solution bags administered to patients by medical professionals.

ASSEMBLY (REFER TO PICTURE AT RIGHT)

Unpacking

Remove the components from the carton:


Qty	Description
1	Adjustable rod set with clutch collar
1	Base star connector
5	Base leg with bolt
1	Base bolt and flat washer
1	IV hook assembly (ram's horns)
1	Tool set: one each M8 hex key & M6 hex key

Assemble base star connector and base legs

1. Install base leg in base star connector.
2. Install base leg screw into base bolt to secure base leg to base star connector. Use M6 hex key to tighten.
3. Repeat steps 1 and 2 for other four base legs.

Assemble IV holder

1. Install adjustable rod in center of base as shown at right.
2. Install flat washer on base screw; install base screw through base into lower rod set. Use M8 hex key to tighten.
3. Install IV hook assembly (ram's horns) on top of adjustable rod set.

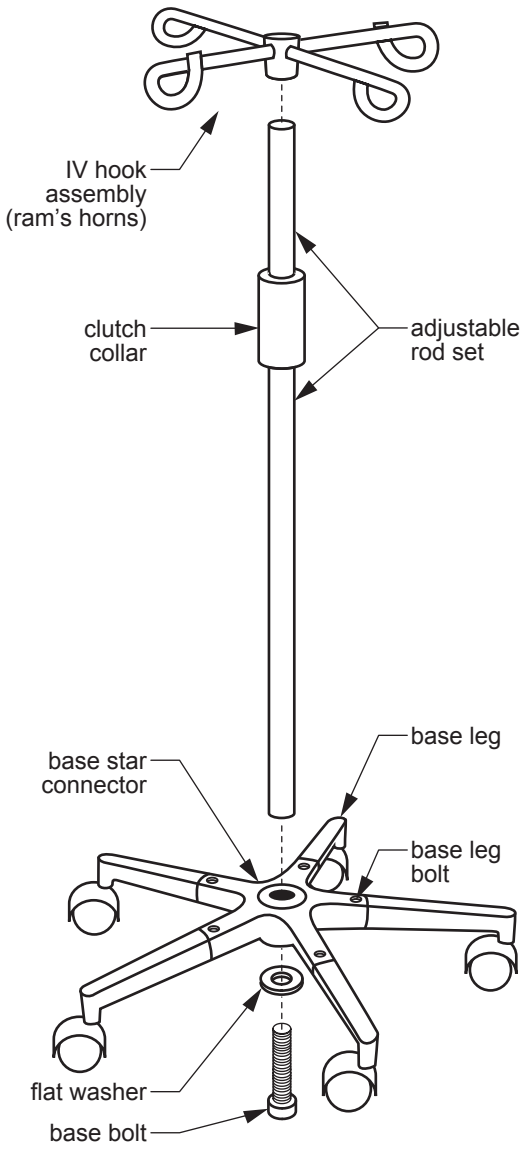

HEIGHT ADJUSTMENT

1. To adjust height, turn clutch collar counter-clockwise until upper rod is loose.
2. Adjust upper rod to desired height.
3. Turn clutch collar clockwise to tighten. DO NOT OVERTIGHTEN.

MAINTENANCE AND CLEANING

To clean the IV Stand, wash with a clean, soft cloth dampened with soap and water or a mild household detergent, wipe with a clean, soft cloth dampened with clear water, and dry with a clean, soft cloth.

⚠ **WARNING: Inspect IV Stand before each use and tighten fasteners as needed to ensure secure installation.**

▲ **NOTICE: Never use abrasive cleaners or scouring pads on any part of the IV Stand.**

LIMITED WARRANTY

SCOPE OF WARRANTY

GF Health Products, Inc. ("GF") warrants to the Original Purchaser only that it will replace or repair components, at GF's sole discretion, that are defective in material or workmanship under normal use and service. All warranties are conditioned upon the proper use of the products strictly in accordance with good commercial practice and applicable GF instructions and manuals, including proper use and maintenance. To the extent that a third party warrants a component, GF conveys all of its rights under that warranty to the Original Purchaser, to the extent permitted. Original Purchaser is one who purchases this product new and unused from GF or a Certified GF Dealer/Distributor. This limited warranty shall only apply to defects that are reported in accordance with the provisions set forth in this warranty document, within the applicable warranty period and which, upon examination by GF or its authorized representative, prove to be a warranty item. (See Obtaining Warranty Service below) This limited warranty is not transferable.

The warranted components and time period are set forth below:

7016A IV Holder ..... 2 (two) years

* Labor is not included in the warranty.

The applicable warranty period shall commence from date of shipment to the Original Purchaser, unless there is an expiration date on the component in which case the warranty shall expire on the earlier of warranty period or the expiration date.

OBTAINING WARRANTY SERVICE

Contact the Dealer/Distributor from whom the product was purchased. If there is not a Dealer/Distributor, you must contact GF directly by calling (770) 368-4700, sending a fax request to 770-368-2386 or by e-mailing a request to cs@grahamfield.com. The Customer Service Representative will provide specific directions. Failure to abide by the specific directions will result in denial of the warranty claim.

The warranty does not cover and GF shall not be liable for the following:

1. Defects, damage, or other conditions caused, in whole or in part, by misuse, abuse, negligence, alteration, accident, freight damage, tampering or failure to seek and obtain repair or replacement in a timely manner;
2. Products which are not installed, used, or properly cleaned and maintained as required in the official manual for the applicable product;
3. Products considered to be of a non-durable nature including, but not limited to: filters, fuses, gaskets, lubricants, and charts;
4. Accessories or parts not provided by GF;
5. Matching of color, grain or texture except to commercially acceptable standards;
6. Changes in color caused by natural or artificial light:
7. Charges by anyone for adjustments, repairs, replacement parts, installation or other work performed upon or in connection with such products which are not expressly authorized in writing, in advance, by GF;
8. Any labor or shipping charges incurred in the replacement part installation or repair;
9. Costs and expenses of regular maintenance and cleaning; and
10. Representations and warranties made by any person or entity other than GF.

ENTIRE WARRANTY, EXCLUSIVE REMEDY AND CONSEQUENTIAL DAMAGES DISCLAIMER

TO THE GREATEST EXTENT PERMITTED BY LAW, THIS WARRANTY IS GF'S ONLY WARRANTY AND IS IN LIEU OF ALL OTHER WARRANTIES, EXPRESS OR IMPLIED. EXCEPT IN CASES WHERE IMPLIED WARRANTIES MAY NOT BE VALIDLY WAIVED, GF MAKES NO IMPLIED WARRANTIES OF ANY KIND INCLUDING ANY IMPLIED WARRANTIES OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE. IF ANY MODEL OR SAMPLE WAS SHOWN TO THE CUSTOMER, SUCH MODEL OR SAMPLE WAS USED MERELY TO ILLUSTRATE THE GENERAL TYPE AND QUALITY OF THE PRODUCT AND NOT TO REPRESENT THAT THE PRODUCT WOULD NECESSARILY CONFORM TO THE MODEL OR SAMPLE IN ALL RESPECTS. THIS WARRANTY IS LIMITED TO THE REPAIR OR REPLACEMENT OF THE DEFECTIVE PARTS. GF SHALL NOT BE LIABLE FOR AND HEREBY DISCLAIMS ANY DIRECT, SPECIAL, INDIRECT, INCIDENTAL, EXEMPLARY OR CONSEQUENTIAL DAMAGES, INCLUDING, BUT NOT LIMITED TO: DAMAGES FOR LOSS OF PROFITS OR INCOME, LOSS OF USE, DOWNTIME, COVER, OR EMPLOYEE OR INDEPENDENT CONTRACTOR WAGES, PAYMENTS AND BENEFITS. CERTAIN STATES AND COUNTRIES MAY CONFER ADDITIONAL RIGHTS REGARDING WARRANTIES AND IN THOSE INSTANCES, GF'S LIABILITY AND THE LIABILITY OF GF'S SUPPLIERS, SHALL BE LIMITED TO THE FULLEST EXTENT PERMITTED BY LAW.

The warranties contained herein, together with GF's current Terms and Conditions, contain all the representations and warranties with respect to the subject matter of this document, and supersede all prior negotiations, agreements and understandings with respect thereto. The recipient of this document hereby acknowledges and represents that it has not relied on any representation, assertion, guarantee, warranty, collateral contract or other assurance, except those set out in this document.

For additional information on this product or this warranty, please contact a GF Customer Service Representative.

NOTES:

1. Additional terms and conditions may apply. See GF's General Terms and Conditions on its website: www.grahamfield.com.
2. Freight claims must be notated on the appropriate shipping documents and must be made with immediacy. International, federal and state regulations govern specific requirements for freight claims. Failure to abide by those regulations may result in a denial of the freight claim. GF will assist you in filing the freight claim.
3. Claims for any short shipment must be made within three (3) days of the invoice date.

LUMEX® by graham-field

Manufactured For:
GF Health Products, Inc.
1 Graham Field Way, Atlanta, GA 30340
Country of origin: India

© 2012, GF Health Products, Inc. All Rights Reserved.
Lumex is a registered trademark of GF Health Products, Inc.

LX_7016A-INS-LAB-RevB26

+1 770.368.4700

Information contained herein is subject to change without notice.
The most current and complete product information can be found on our website.

www.grahamfield.com

graham field™